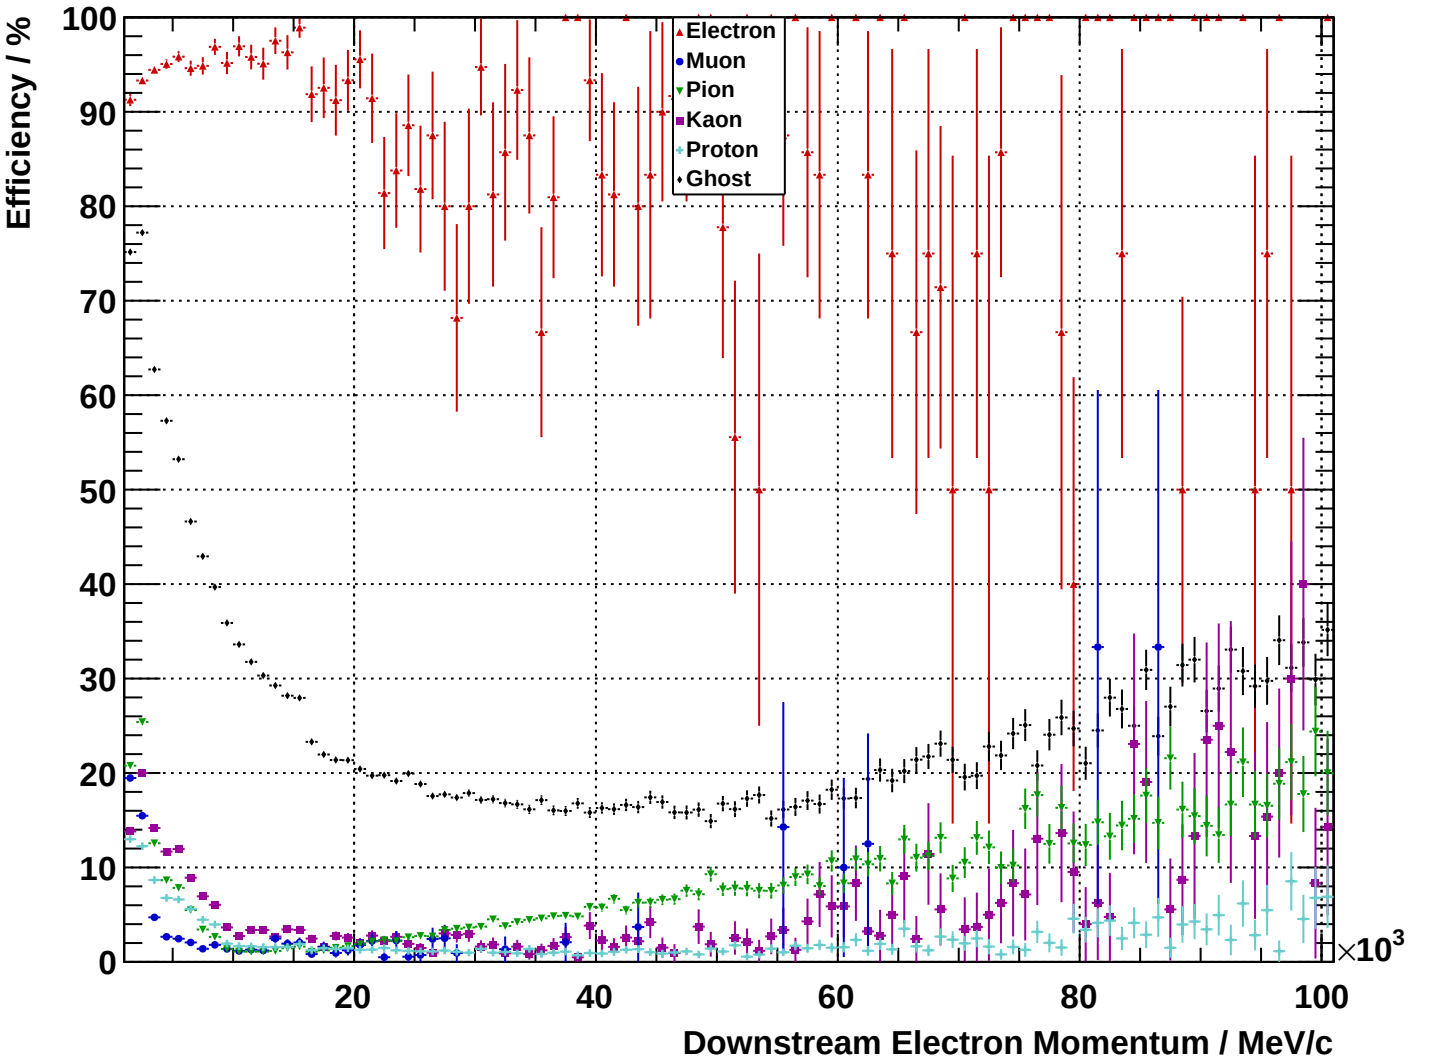Downstream Electron ID Eff. V TrackP | MVAout > 0.1000 | MLP Norm BP NCycles750 CE sigmoid HL1SF1.6 HL2SF1.2 CVTest15:1e-16 !UseReg
All EqualSigBck:0.1 AllPhysTracksInEvent:AllPhysTracksInEvent NoReweight EvalWithPreSel | Train:UpgradeSim09cUp02RecoUp01MixtureGhosts GhF0.001 Eval:UpgradeSim09cUp02RecoUp01MixtureGhosts | TMVA-Upgrade-Sim09cUp02RecoUp01