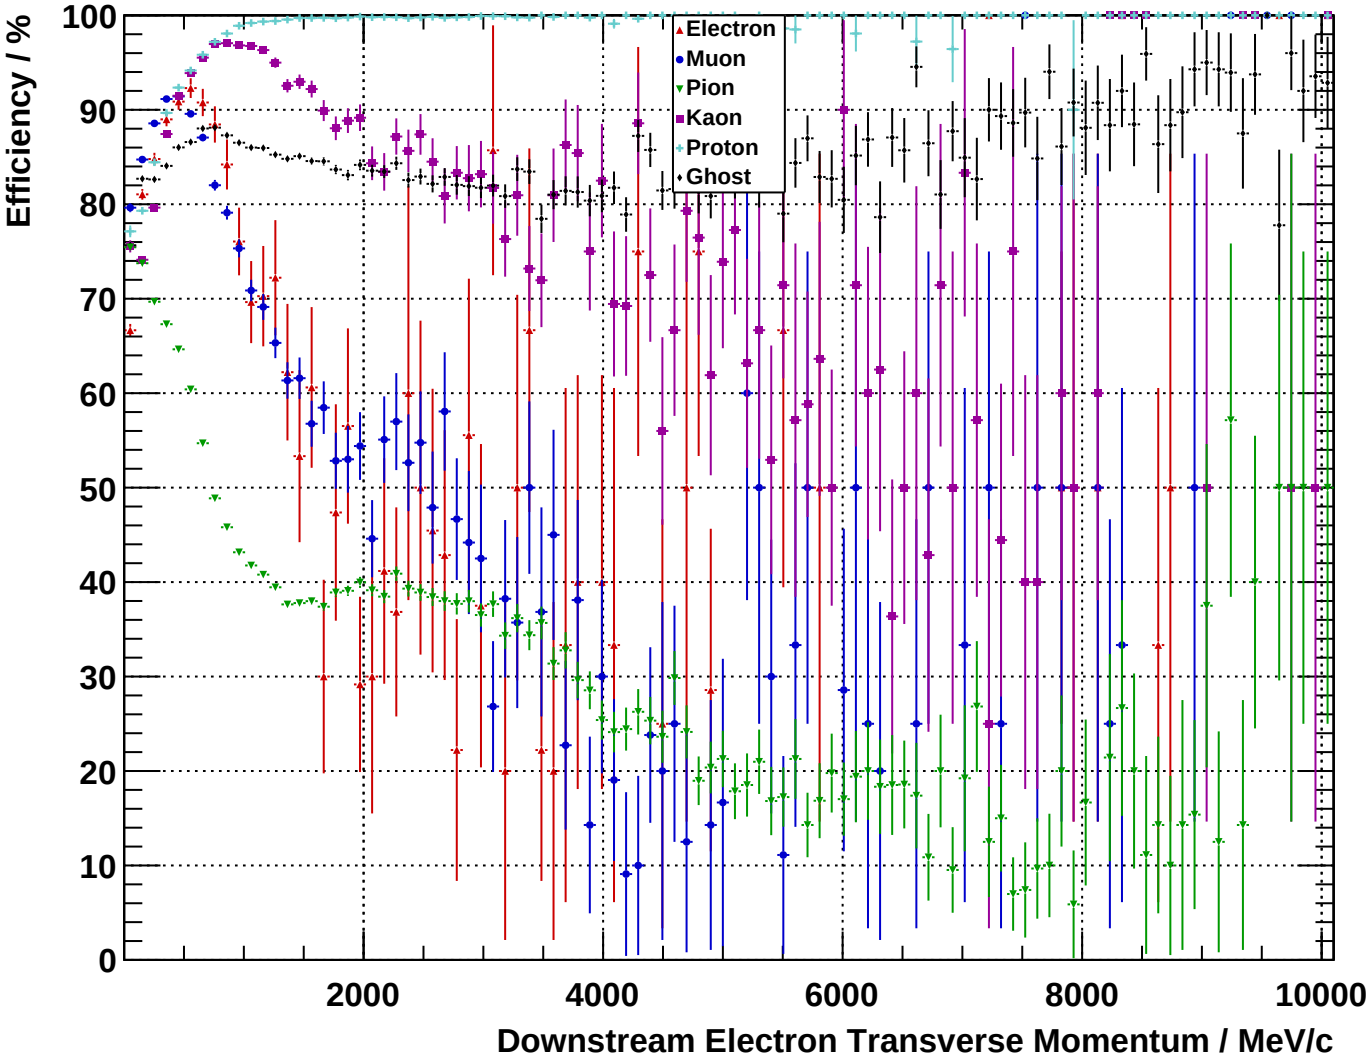Downstream Electron ID Eff. V TrackPt | CombDLLp > -2.0000 | MLP Norm BP NCycles750 CE sigmoid HL1SF1.6 HL2SF1.6 CVTest15:1e-16 !UseReg
All NaturalMix AllPhysTracksInEvent:AllPhysTracksInEvent NoReweight EvalWithPreSel | Train:UpgradeSim09cUp02RecoUp01MixtureGhosts GhF0.1 KaF0.1 Eval:UpgradeSim09cUp02RecoUp01MixtureGhosts | TMVA-Upgrade-Sim09cUp02RecoUp01